



Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	NovaLabs




Sample

Retatrutide 10mg
NovaLabs

RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1 10mg	May 2026	99.78%	11.18 mg

#1 UV CHROMATOGRAM

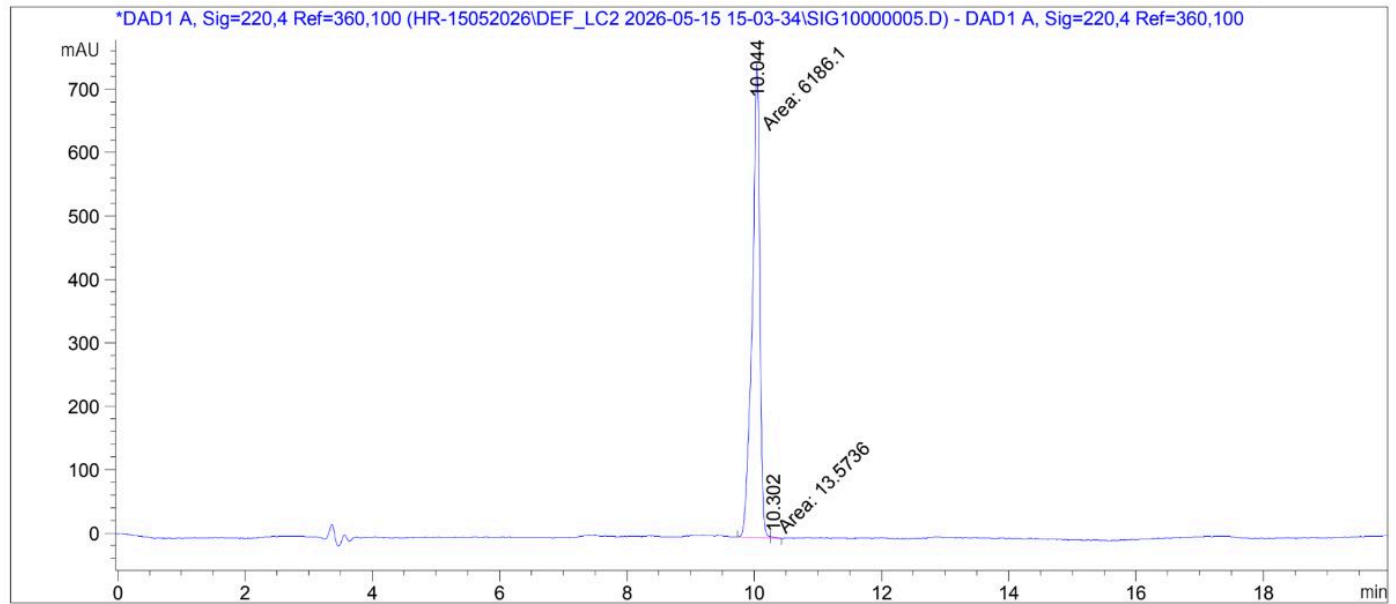

COMMENT

ANALYSIS CONDUCTED

15 MAY 2026

ZAGREB, CROATIA (EU)

Alex Mihaljcic
DIRECTOR

